


Chromatogram and Results

Injection Details

Injection Name:	MK2866; BA33901	Run Time (min):	25.00
Vial Number:		Injection Volume:	10.00
Injection Type:	Unknown	Channel:	EXT197NM
Calibration Level:		Wavelength:	n.a.
Instrument Method:	AD 250mm MaxRP 25min Purity Method	Bandwidth:	n.a.
Processing Method:	Processing Method	Dilution Factor:	1.0000
Injection Date/Time:	18/May/25 12:36	Sample Weight:	1.0000

Chromatogram

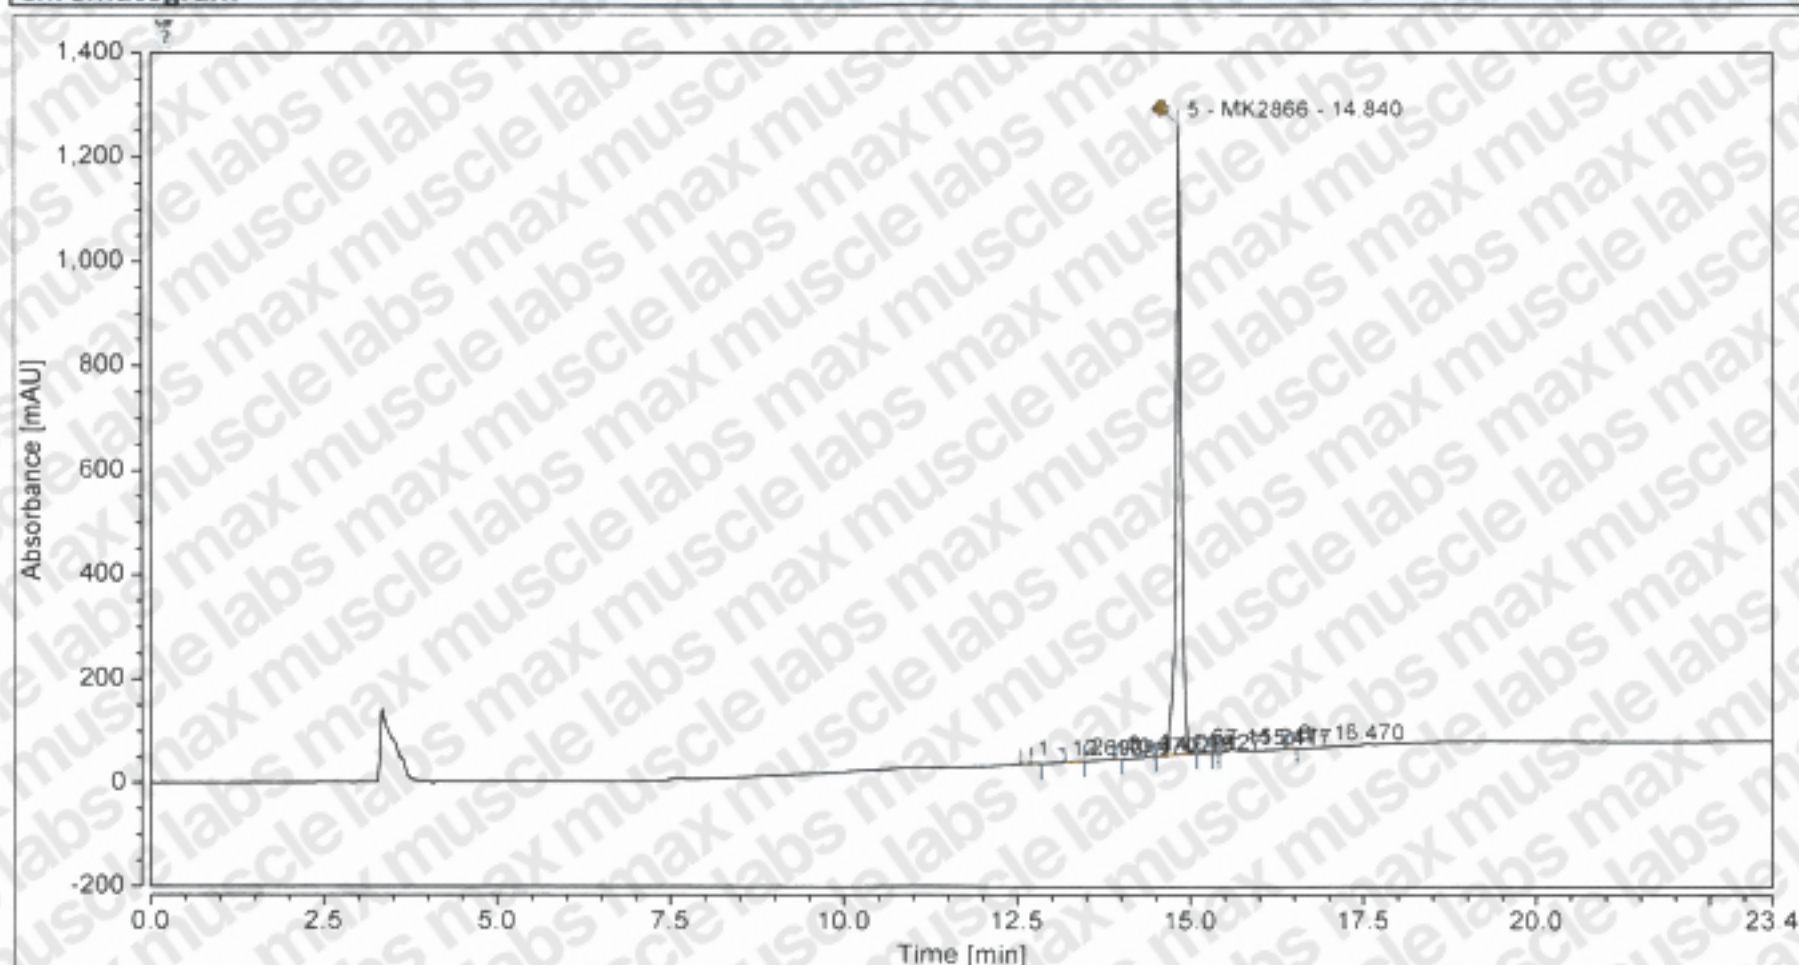

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
1		12.693	0.210	2.486	0.19	0.20	n.a.
2		13.470	0.094	0.000	0.09	0.00	n.a.
3		14.010	0.011	0.000	0.01	0.00	n.a.
4		14.427	0.047	0.722	0.04	0.06	n.a.
5	MK2866	14.840	108.098	1206.585	99.35	99.33	n.a.
6		15.217	0.241	3.525	0.22	0.29	n.a.
7		15.417	0.009	0.000	0.01	0.00	n.a.
8		16.470	0.096	1.372	0.09	0.11	n.a.
Total:			108.806	1214.691	100.00	100.00	