


Chromatogram and Results

Injection Details

Injection Name:	MK677; BA34001	Run Time (min):	25.00
Vial Number:		Injection Volume:	10.00
Injection Type:	Unknown	Channel:	UV_VIS_1
Calibration Level:		Wavelength:	195
Instrument Method:	AD 250mm MaxRP 25min Purity Method	Bandwidth:	5
Processing Method:	Processing Method	Dilution Factor:	1.0000
Injection Date/Time:	14/Mar/25 22:46	Sample Weight:	1.0000

Chromatogram

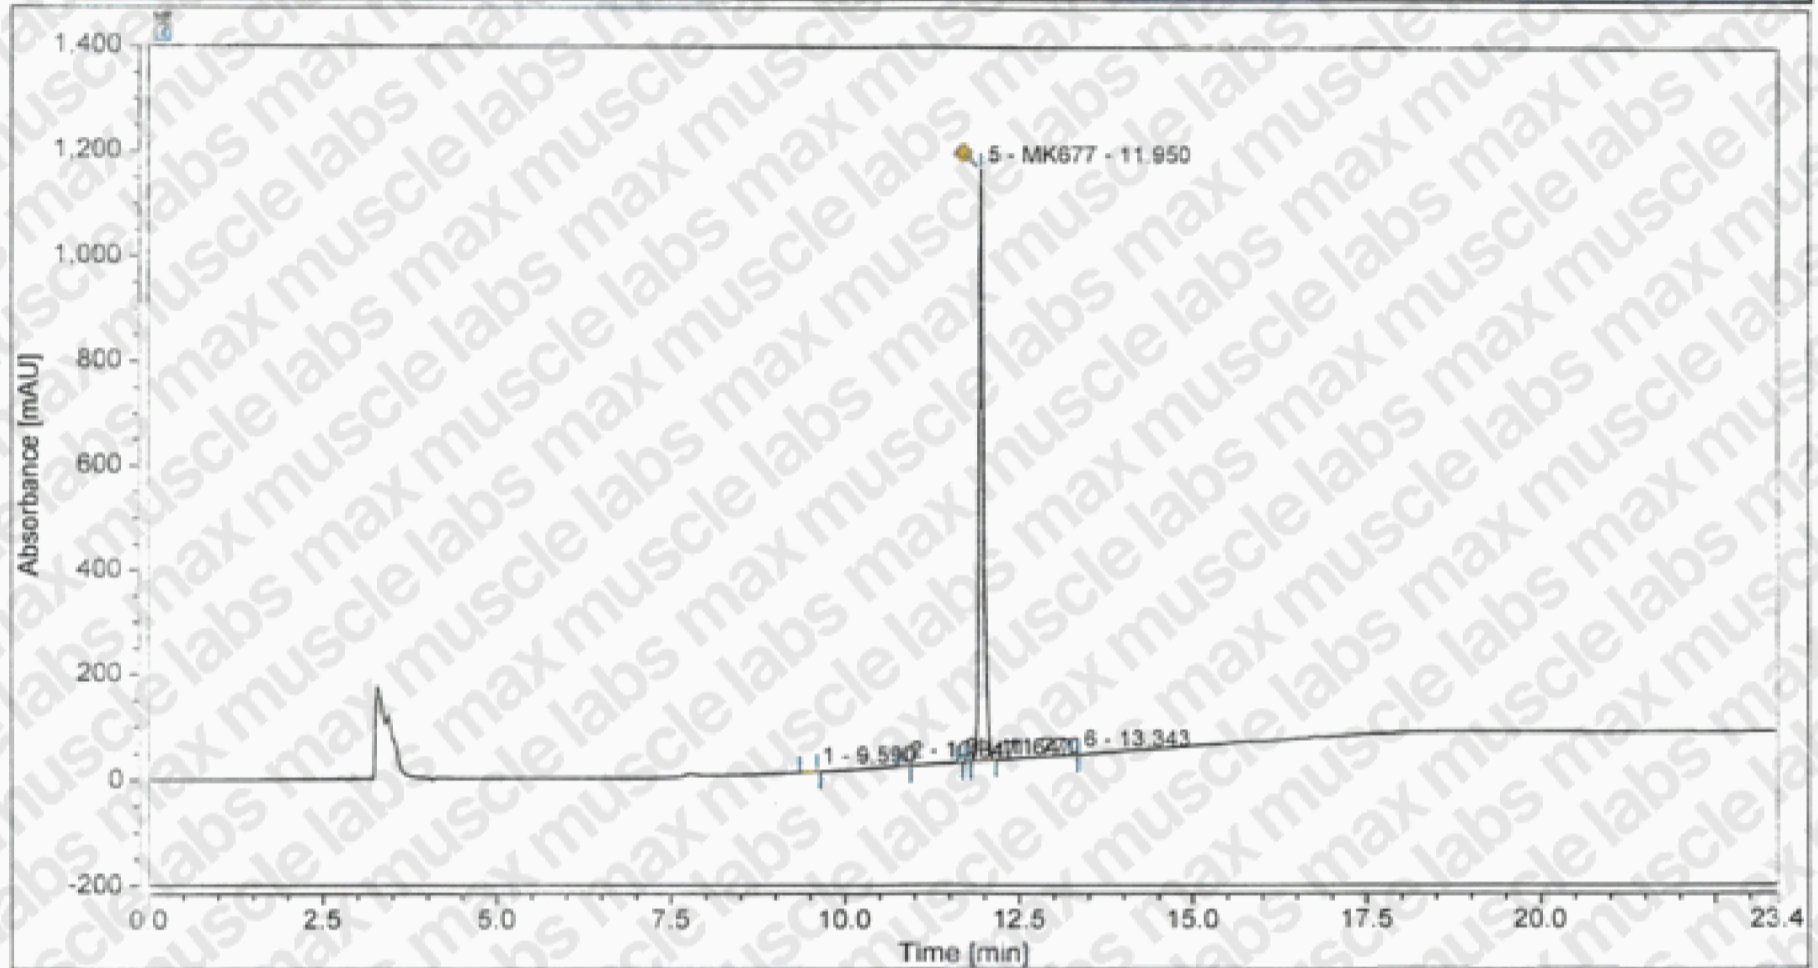

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
1		9.590	0.155	1.810	0.19	0.16	n.a.
2		10.847	0.060	0.820	0.07	0.07	n.a.
3		11.647	0.013	0.294	0.02	0.03	n.a.
4		11.770	0.019	0.449	0.02	0.04	n.a.
5	MK677	11.950	80.058	1130.650	99.67	99.70	n.a.
6		13.343	0.018	0.000	0.02	0.00	n.a.
Total:			80.324	1134.022	100.00	100.00	