


Chromatogram and Results

Injection Details

Injection Name:	RAD140; BA34101	Run Time (min):	20.00
Vial Number:		Injection Volume:	10.00
Injection Type:	Unknown	Channel:	EXT278NM
Calibration Level:		Wavelength:	n.a.
Instrument Method:	AD 150mm MaxRP 20min	Bandwidth:	n.a.
Processing Method:	Processing Method	Dilution Factor:	1.0000
Injection Date/Time:	27/Apr/25 15:26	Sample Weight:	1.0000

Chromatogram

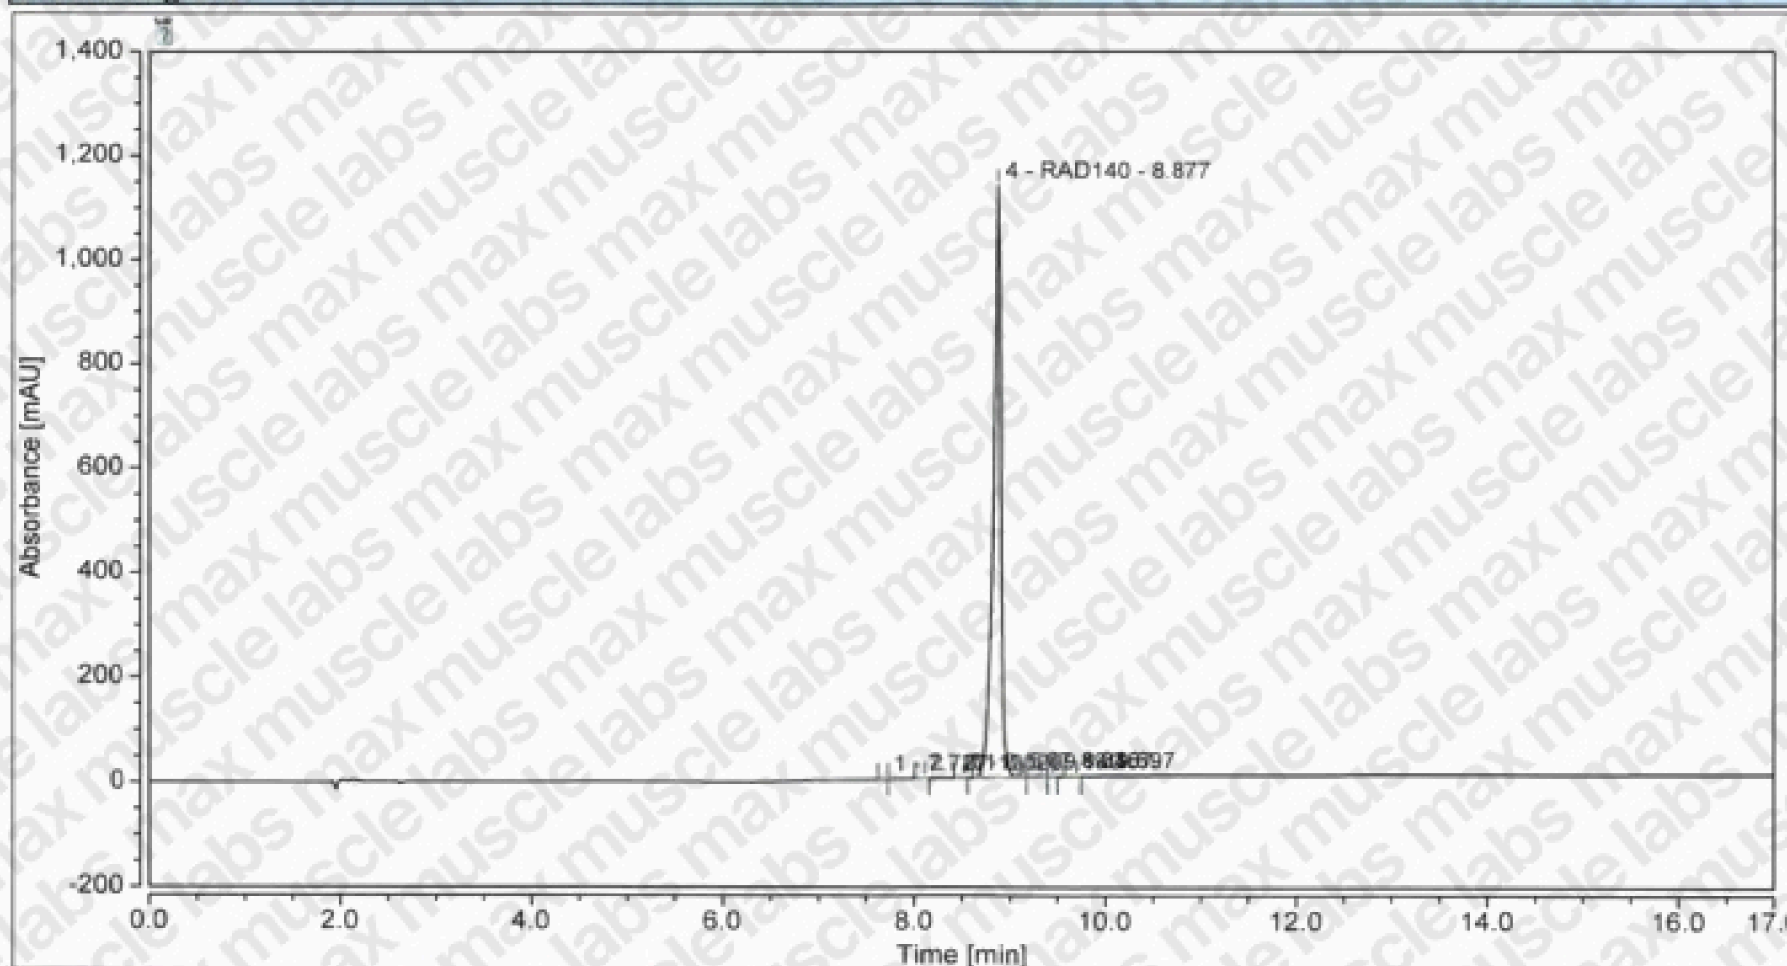

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
1		7.727	0.005	0.000	0.01	0.00	n.a.
2		8.113	0.016	0.253	0.02	0.02	n.a.
3		8.520	0.011	0.117	0.01	0.01	n.a.
4	RAD140	8.877	98.888	1133.804	99.77	99.71	n.a.
5		9.140	0.006	0.152	0.01	0.01	n.a.
6		9.330	0.142	1.984	0.14	0.17	n.a.
7		9.457	0.016	0.337	0.02	0.03	n.a.
8		9.697	0.028	0.419	0.03	0.04	n.a.
Total:			99.112	1137.066	100.00	100.00	