


Chromatogram and Results

Injection Details			
Injection Name:	RAD150 BA34601	Run Time (min):	25.00
Vial Number:		Injection Volume:	10.00
Injection Type:	Unknown	Channel:	EXT276NM
Calibration Level:		Wavelength:	195.0
Instrument Method:	AD MaxRP Gradient 25m	Bandwidth:	4
Processing Method:	Processing Method	Dilution Factor:	1.0000
Injection Date/Time:	04/Nov/25 18:50	Sample Weight:	1.0000

Chromatogram

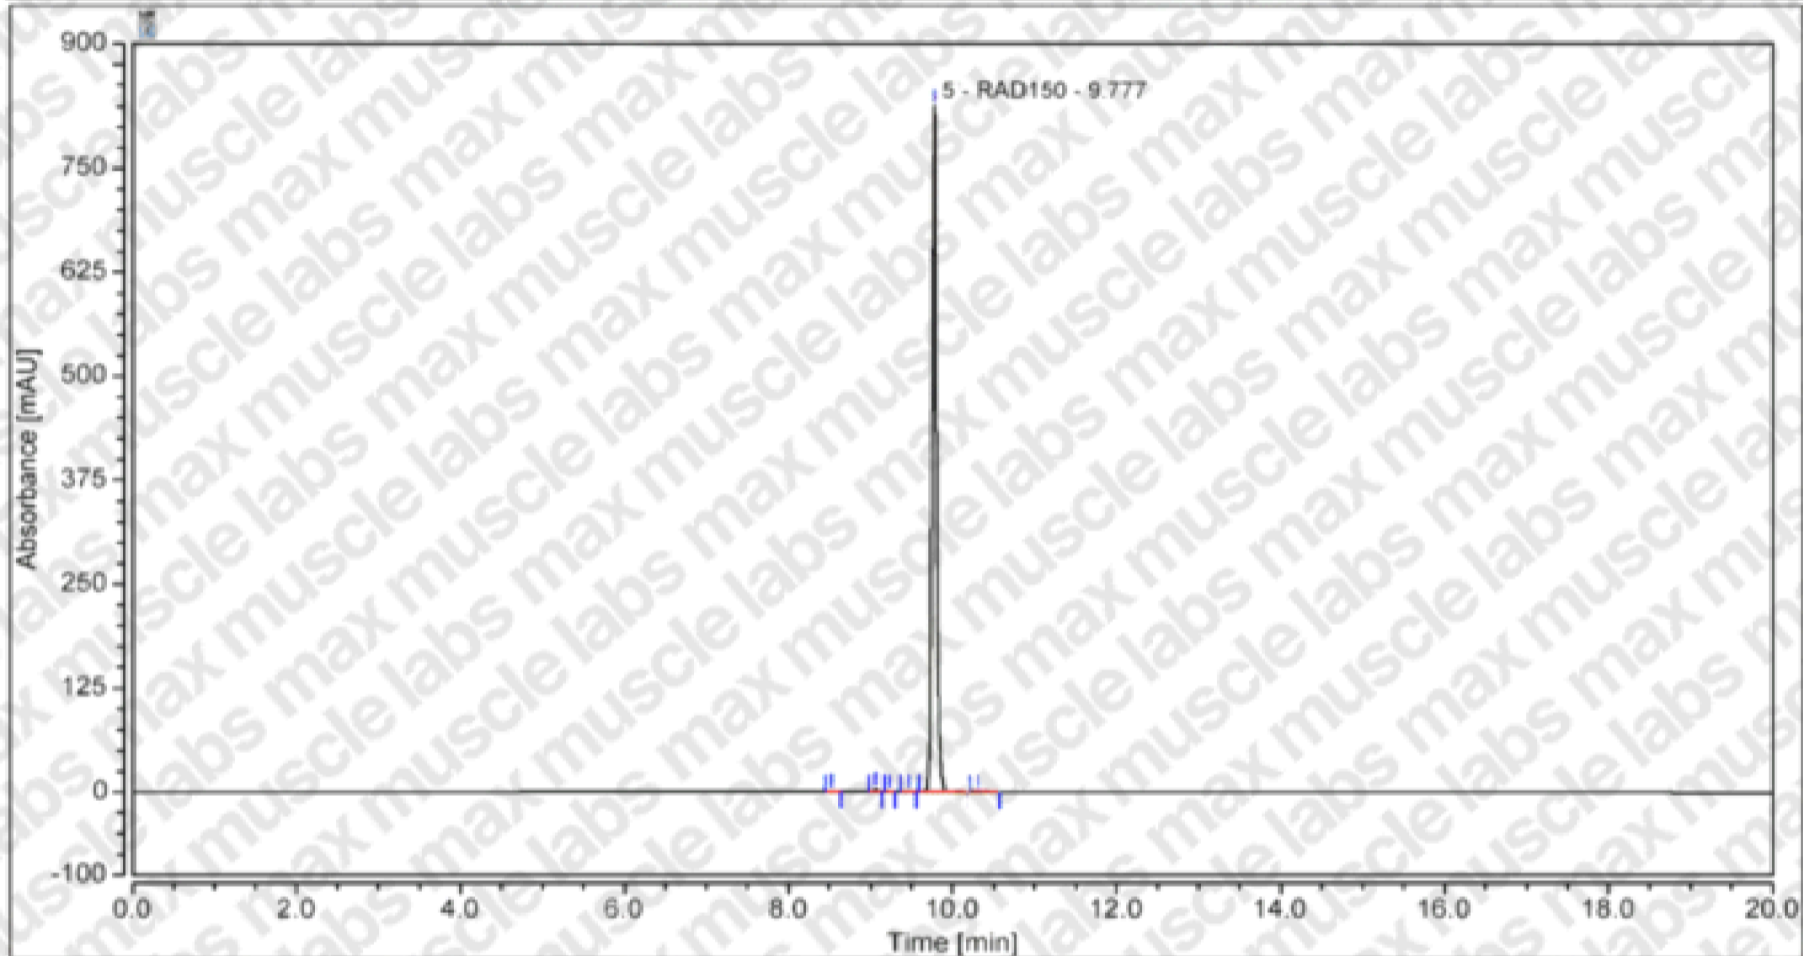

Integration Results							
No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount µg/ml
1		8.523	0.051	0.959	0.10	0.12	n.a.
2		9.060	0.169	3.445	0.32	0.41	n.a.
3		9.233	0.030	0.565	0.06	0.07	n.a.
4		9.470	0.022	0.249	0.04	0.03	n.a.
5	RAD150	9.777	52.813	824.919	99.31	99.23	n.a.
6		10.313	0.098	1.170	0.18	0.14	n.a.
Total:			53.182	831.307	100.00	100.00	