


### Chromatogram and Results

#### Injection Details

Injection Name:	SR9009 lot BA34901	Run Time (min):	25.00
Vial Number:		Injection Volume:	10.00
Injection Type:	Unknown	Channel:	UV_VIS_1
Calibration Level:		Wavelength:	195
Instrument Method:	AD 250mm MaxRP 25min Purity Method	Bandwidth:	5
Processing Method:	Processing Method	Dilution Factor:	1.0000
Injection Date/Time:	14/Mar/25 15:21	Sample Weight:	1.0000

#### Chromatogram

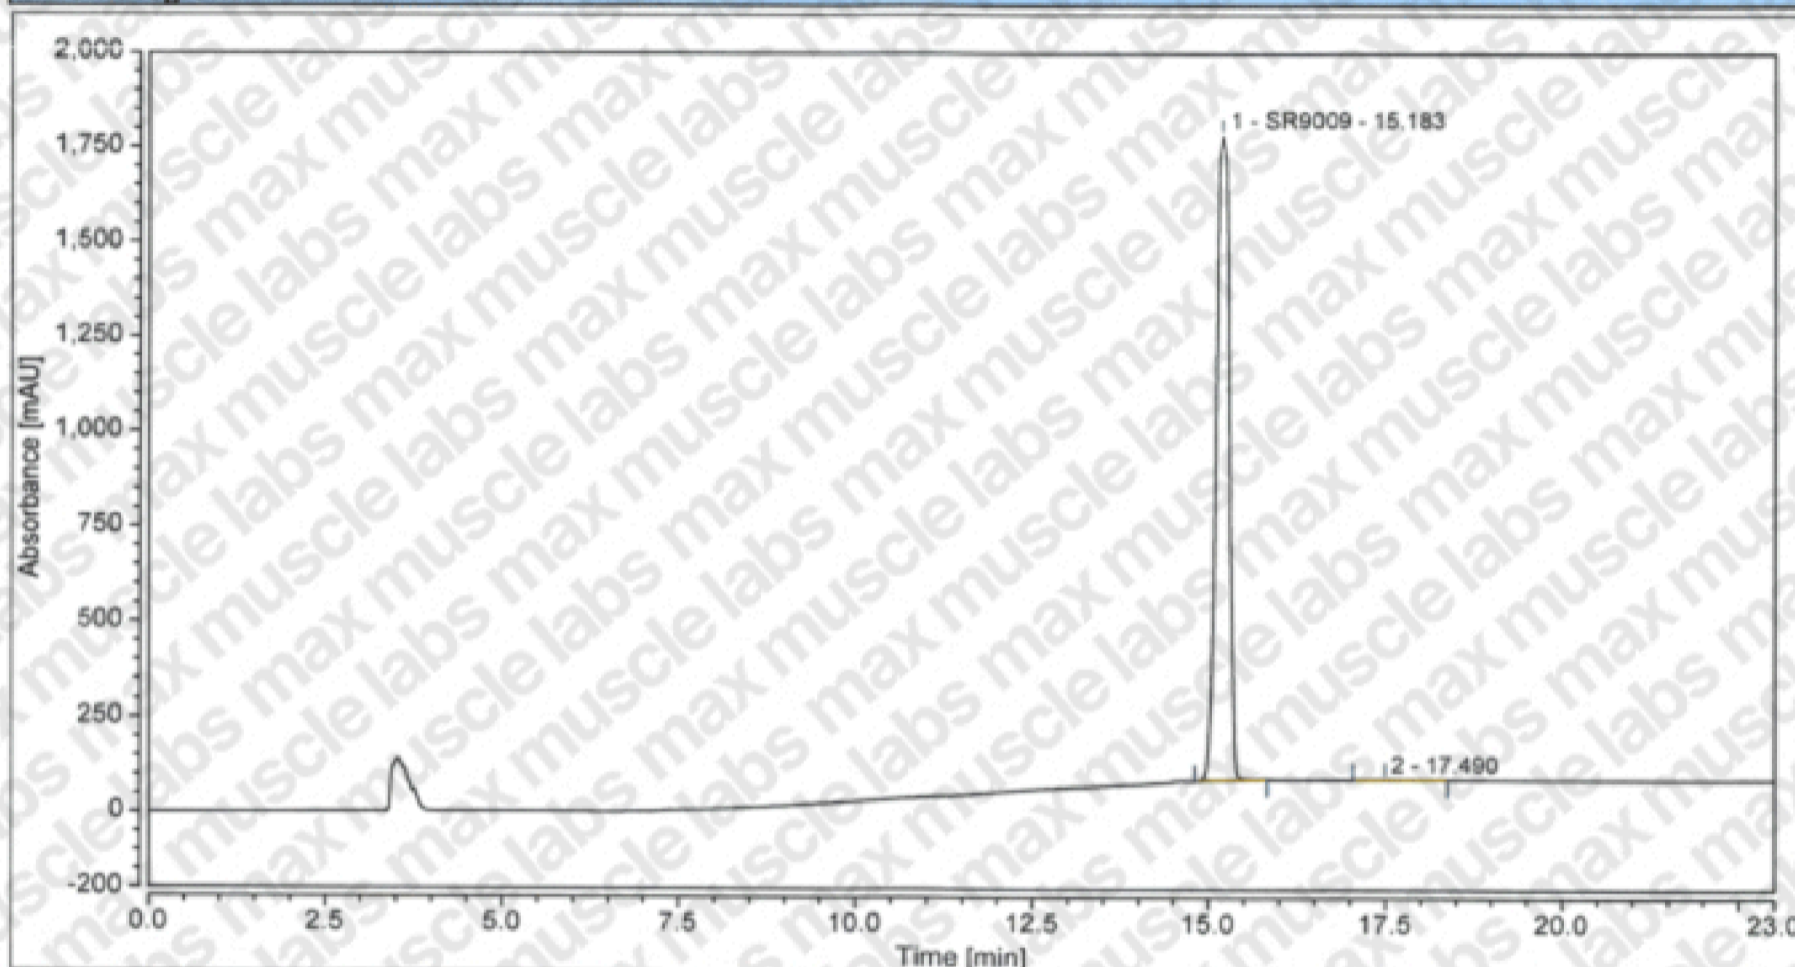

#### Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
1	SR9009	15.183	359.186	1694.160	99.84	99.95	n.a.
2		17.490	0.576	0.848	0.16	0.05	n.a.
<b>Total:</b>			<b>359.762</b>	<b>1695.007</b>	<b>100.00</b>	<b>100.00</b>	