


### Chromatogram and Results

#### Injection Details

Injection Name:	SR9011 BA35501	Run Time (min):	25.00
Vial Number:		Injection Volume:	10.00
Injection Type:	Unknown	Channel:	EXT220NM
Calibration Level:		Wavelength:	n.a.
Instrument Method:	AD 250mm MaxRP 25min Purity Method	Bandwidth:	n.a.
Processing Method:	Processing Method	Dilution Factor:	1.0000
Injection Date/Time:	04/Nov/25 18:50	Sample Weight:	1.0000

#### Chromatogram

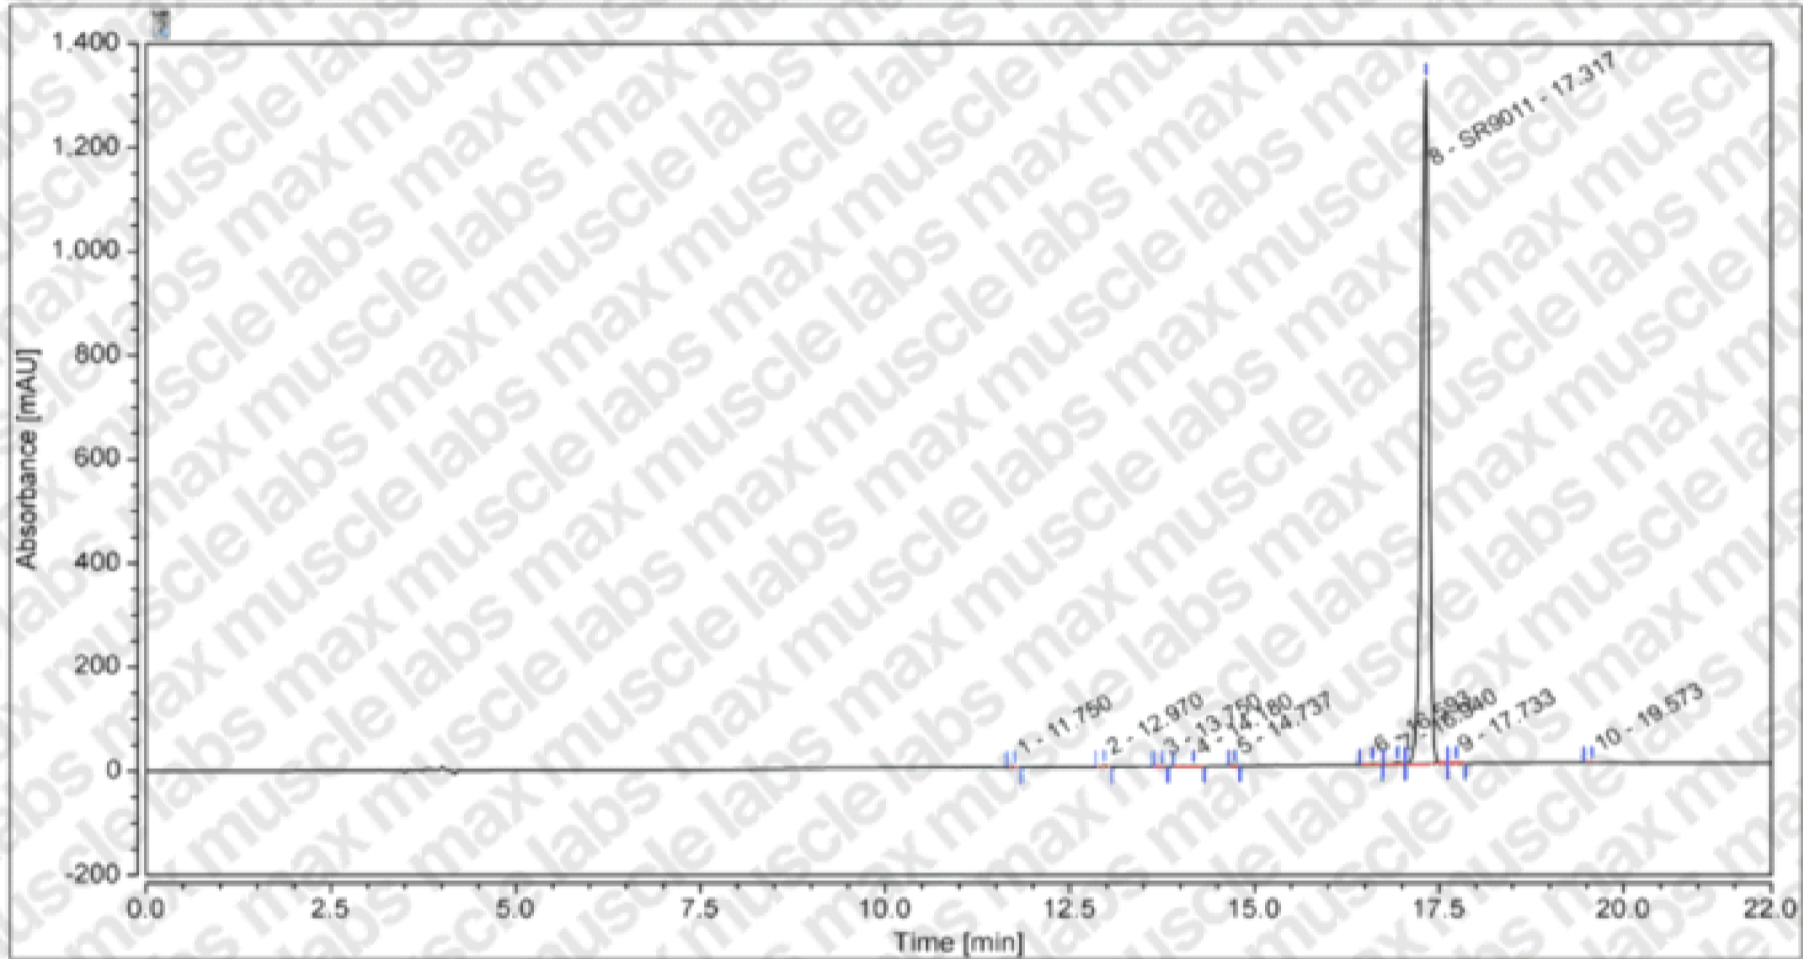

#### Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
1		11.750	0.042	0.513	0.03	0.04	n.a.
2		12.970	0.171	2.150	0.11	0.16	n.a.
3		13.750	0.053	0.481	0.03	0.04	n.a.
4		14.180	0.202	0.993	0.13	0.07	n.a.
5		14.737	0.021	0.250	0.01	0.02	n.a.
6		16.593	0.263	2.358	0.17	0.18	n.a.
7		16.940	0.354	3.495	0.23	0.26	n.a.
8	SR9011	17.317	150.391	1316.105	99.13	99.08	n.a.
9		17.733	0.171	1.611	0.11	0.12	n.a.
10		19.573	0.045	0.405	0.03	0.03	n.a.
Total:			151.712	1328.361	100.00	100.00	